




JDENTAL CARE  
*just smile*

# JD EVOLUTION plus

*Simple insertion, natural stability*



hexagonal connection




Made in Italy

# SIMPLE INSERTION, NATURAL STABILITY

## features & advantages

- Internal hex connection with lead-in bevel
- Anatomic coronal collar
- Expanding tapered inner body
- Self-cutting capacity in both directions
- Apical cutting blades
- The connection is universally recognized by all the main digital libraries
- Reduces stress concentration on the crestal bone and maximizes bone volume around the implant neck for stable hard and soft tissues
- Makes it possible to achieve high primary stability

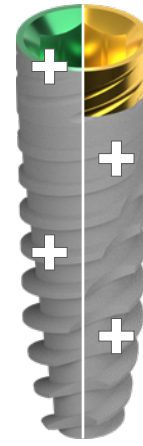


Full SLA surface treatment

H 1,5mm anodised implant collar and SLA surface treatment on the body

## SINGLE PROSTHETIC CONNECTION

Single prosthetic connection for all diameters  
Reduced inventory and enhanced working flexibility

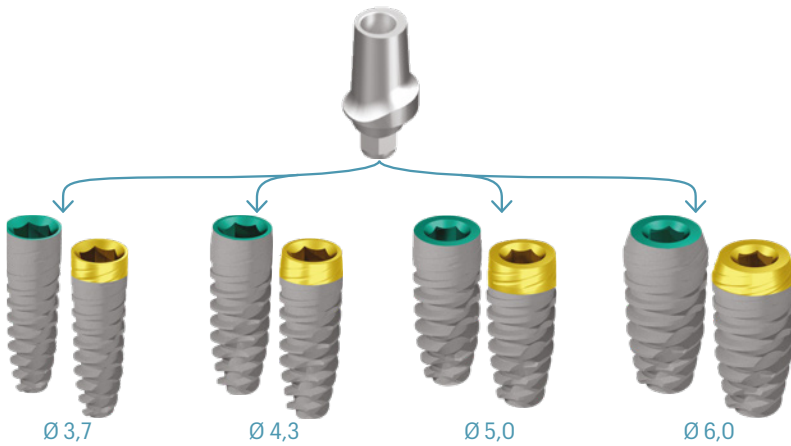


## PRODUCT SPECIFICATIONS

Note: All measurements in mm

The JDEvolution Plus dental implants are available in the diameters and lengths shown in the following table:

IMPLANT DIAMETER	LENGTH	TIP DIAMETER	PLATFORM DIAMETER	ABUTMENT INTERFACE
Ø 3.7	8	2.8	3.7	3.4
	10, 11.5, 13, 15, 18	2.4		
Ø 4.0	6	3.5	4.0	3.4
	8	2.8		
	10	2.5		
	11.5, 13	2.4		
Ø 4.3	6	3.82	4.0	3.4
	8	3.55		
	10, 11.5, 13, 15, 18	2.8		
Ø 5.0	6	3.85	4.8	3.4
	8, 10, 11.5, 13, 15	3.2		
Ø 6.0	6	4.4	5.0	3.4
	8	4.1		
	10, 11.5, 13, 15	4		

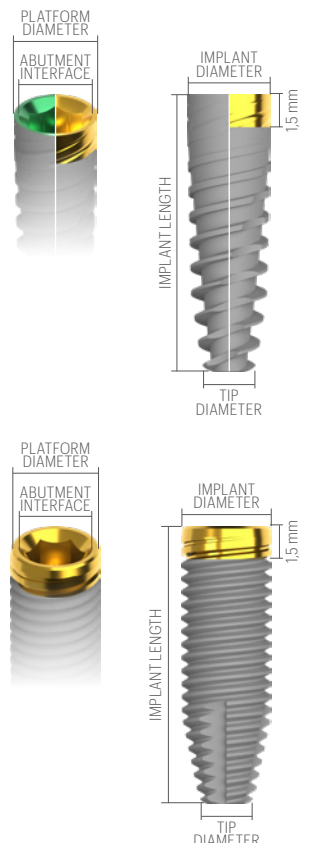

The JDEvolution Plus T dental implants are available in the diameters and lengths shown in the following table:

IMPLANT DIAMETER	LENGTH	TIP DIAMETER	PLATFORM DIAMETER	ABUTMENT INTERFACE
Ø 4.0	6	2.6	3.8	3.4
	8, 10, 11.5, 13, 15, 18	2.4		

# PRODUCT CATALOGUE

Note: all measurements of diameters and lengths are in mm

## Implants:

### Ø 3,7

EV37080:	JDEvolution Plus Ø 3.7 L 8
EV37100:	JDEvolution Plus Ø 3.7 L 10
EV37115:	JDEvolution Plus Ø 3.7 L 11.5
EV37130:	JDEvolution Plus Ø 3.7 L 13
EV37150:	JDEvolution Plus Ø 3.7 L 15
EV37180:	JDEvolution Plus Ø 3.7 L 18

### Ø 4,0

EV40060:	JDEvolution Plus Ø 4.0 L 6
EV40080:	JDEvolution Plus Ø 4.0 L 8
EV40100:	JDEvolution Plus Ø 4.0 L 10
EV40115:	JDEvolution Plus Ø 4.0 L 11.5
EV40130:	JDEvolution Plus Ø 4.0 L 13

### Ø 4,3


EV43060:	JDEvolution Plus Ø 4.3 L 6
EV43080:	JDEvolution Plus Ø 4.3 L 8
EV43100:	JDEvolution Plus Ø 4.3 L 10
EV43115:	JDEvolution Plus Ø 4.3 L 11.5
EV43130:	JDEvolution Plus Ø 4.3 L 13
EV43150:	JDEvolution Plus Ø 4.3 L 15
EV43180:	JDEvolution Plus Ø 4.3 L 18

### Ø 5,0

EV50060:	JDEvolution Plus Ø 5.0 L 6
EV50080:	JDEvolution Plus Ø 5.0 L 8
EV50100:	JDEvolution Plus Ø 5.0 L 10
EV50115:	JDEvolution Plus Ø 5.0 L 11.5
EV50130:	JDEvolution Plus Ø 5.0 L 13
EV50150:	JDEvolution Plus Ø 5.0 L 15
EV50180:	JDEvolution Plus Ø 5.0 L 18

### Ø 6,0

EV60060:	JDEvolution Plus Ø 6.0 L 6
EV60080:	JDEvolution Plus Ø 6.0 L 8
EV60100:	JDEvolution Plus Ø 6.0 L 10
EV60115:	JDEvolution Plus Ø 6.0 L 11.5
EV60130:	JDEvolution Plus Ø 6.0 L 13
EV60150:	JDEvolution Plus Ø 6.0 L 15

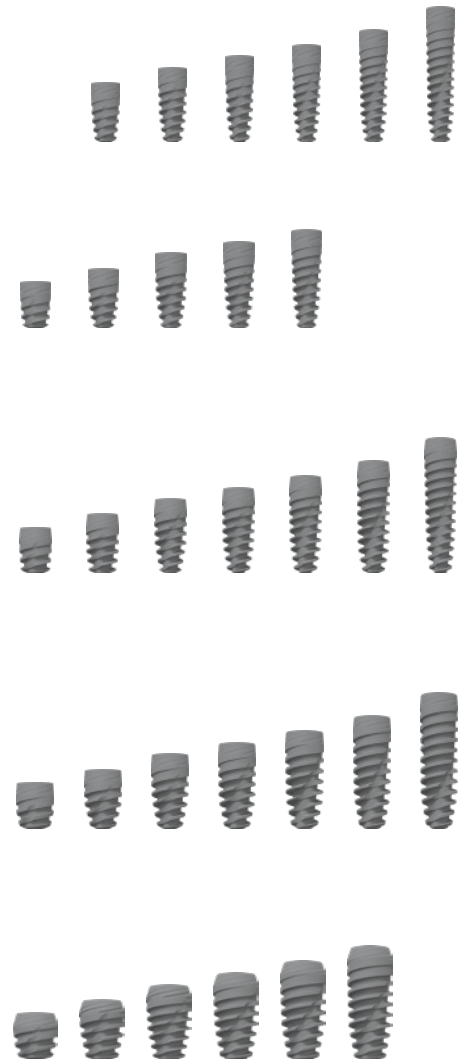

## Anodised implant collar:

### Ø 3,7


EVA37080:	JDEvolution Plus Anodized Collar Ø 3.7 L 8
EVA37100:	JDEvolution Plus Anodized Collar Ø 3.7 L 10
EVA37115:	JDEvolution Plus Anodized Collar Ø 3.7 L 11.5
EVA37130:	JDEvolution Plus Anodized Collar Ø 3.7 L 13
EVA37150:	JDEvolution Plus Anodized Collar Ø 3.7 L 15
EVA37180:	JDEvolution Plus Anodized Collar Ø 3.7 L 18

### Ø 4,0

EVA40150:	JDEvolution Plus Anodized Collar Ø 4.0 L 15
EVA40180:	JDEvolution Plus Anodized Collar Ø 4.0 L 18

### Ø 4,3

EVA43060:	JDEvolution Plus Anodized Collar Ø 4.3 L 6
EVA43080:	JDEvolution Plus Anodized Collar Ø 4.3 L 8
EVA43100:	JDEvolution Plus Anodized Collar Ø 4.3 L 10
EVA43115:	JDEvolution Plus Anodized Collar Ø 4.3 L 11.5
EVA43130:	JDEvolution Plus Anodized Collar Ø 4.3 L 13
EVA43150:	JDEvolution Plus Anodized Collar Ø 4.3 L 15
EVA43180:	JDEvolution Plus Anodized Collar Ø 4.3 L 18

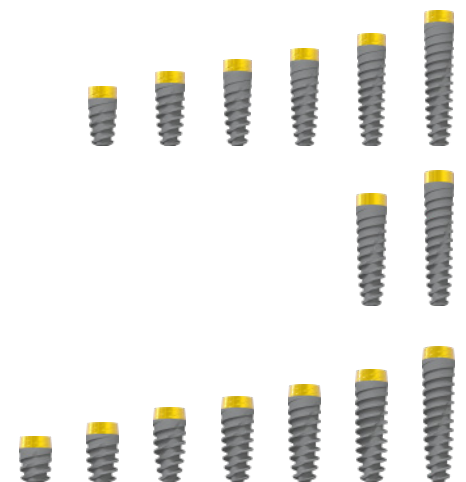

### Ø 5,0

EVA50060:	JDEvolution Plus Anodized Collar Ø 5.0 L 6
EVA50080:	JDEvolution Plus Anodized Collar Ø 5.0 L 8
EVA50100:	JDEvolution Plus Anodized Collar Ø 5.0 L 10
EVA50115:	JDEvolution Plus Anodized Collar Ø 5.0 L 11.5
EVA50130:	JDEvolution Plus Anodized Collar Ø 5.0 L 13
EVA50150:	JDEvolution Plus Anodized Collar Ø 5.0 L 15
EVA50180:	JDEvolution Plus Anodized Collar Ø 5.0 L 18



### Ø 6,0

EVA60060:	JDEvolution Plus Anodized Collar Ø 6.0 L 6
EVA60080:	JDEvolution Plus Anodized Collar Ø 6.0 L 8
EVA60100:	JDEvolution Plus Anodized Collar Ø 6.0 L 10
EVA60115:	JDEvolution Plus Anodized Collar Ø 6.0 L 11.5
EVA60130:	JDEvolution Plus Anodized Collar Ø 6.0 L 13
EVA60150:	JDEvolution Plus Anodized Collar Ø 6.0 L 15



### JDEvolution Plus T:

EVT40060:	JDEvolution Plus T Anodized Collar Ø 4.0 L 6
EVT40080:	JDEvolution Plus T Anodized Collar Ø 4.0 L 8
EVT40100:	JDEvolution Plus T Anodized Collar Ø 4.0 L 10
EVT40115:	JDEvolution Plus T Anodized Collar Ø 4.0 L 11.5
EVT40130:	JDEvolution Plus T Anodized Collar Ø 4.0 L 13
EVT40150:	JDEvolution Plus T Anodized Collar Ø 4.0 L 15
EVT40180:	JDEvolution Plus T Anodized Collar Ø 4.0 L 18



### Cover screw:

EVCS:	Cover Screw JDEvolution Plus
EVCS6:	Cover Screw Ø 6.0 JDEvolution Plus



### Healing Abutment:


EVHA41:	Healing Abutment Ø 4.0 H 1.0 JDEvolution Plus
EVHA42:	Healing Abutment Ø 4.0 H 2.0 JDEvolution Plus
EVHA43:	Healing Abutment Ø 4.0 H 3.0 JDEvolution Plus
EVHA45:	Healing Abutment Ø 4.0 H 5.0 JDEvolution Plus
EVHA47:	Healing Abutment Ø 4.0 H 7.0 JDEvolution Plus
EVHA53:	Healing Abutment Ø 5.0 H 3.0 JDEvolution Plus
EVHA55:	Healing Abutment Ø 5.0 H 5.0 JDEvolution Plus
EVHA57:	Healing Abutment Ø 5.0 H 7.0 JDEvolution Plus
EVHA59:	Healing Abutment Ø 5.0 H 9.0 JDEvolution Plus
EVHA63:	Healing Abutment Ø 6.0 H 3.0 JDEvolution Plus
EVHA65:	Healing Abutment Ø 6.0 H 5.0 JDEvolution Plus
EVHA67:	Healing Abutment Ø 6.0 H 7.0 JDEvolution Plus
EVHA753:	Healing Abutment Ø 7.5 H 3.0 JDEvolution Plus
EVHA755:	Healing Abutment Ø 7.5 H 5.0 JDEvolution Plus
EVHA54TS:	Healing Abutment Tissue Ø 5.0 H 4.0 JDEvolution Plus
EVHA56TS:	Healing Abutment Tissue Ø 5.0 H 6.0 JDEvolution Plus



### Impression coping:

#### OPEN TRAY

EVICOT4C:	Impression Coping Open Tray Ø 4.0 JDEvolution Plus
EVICOT5C:	Impression Coping Open Tray Ø 5.0 JDEvolution Plus
EVICOT6C:	Impression Coping Open Tray Ø 6.0 JDEvolution Plus
EVICOTNEC:	Impression Coping Open Tray Non Engaging JDEvolution Plus
EVICOTS:	Impression Coping Open Tray Screw JDEvolution Plus
EVICOT5TSC:	Impression Coping Tissue Open Tray Ø 5.0 JDEvolution Plus

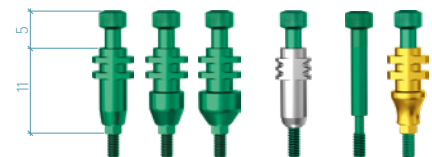

#### CLOSED TRAY


EVICCT4C:	Impression Coping Closed Tray Ø 4.0 JDEvolution Plus
EVICCT5C:	Impression Coping Closed Tray Ø 5.0 JDEvolution Plus
EVICCT6C:	Impression Coping Closed Tray Ø 6.0 JDEvolution Plus
EVICCTS:	Impression Coping Closed Tray Screw JDEvolution Plus
EVICCT1C:	Impression Coping Closed Tray Direct Press Fit JDEvolution Plus



## Temporary Abutment:

EVTAE C:	Temporary Abutment Engaging JDEvolution Plus
EVTAEPC:	Temporary Abutment Engaging Peek JDEvolution Plus
EVTANEC:	Temporary Abutment Non Engaging JDEvolution Plus
EVTAE TSC:	Temporary Abutment Tissue Engaging JDEvolution Plus
EVTANETSC:	Temporary Abutment Tissue Non Engaging JDEvolution Plus

Torque recommended 30 Ncm

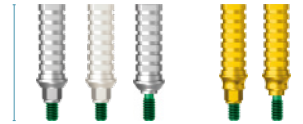


## Straight Abutment:

EVNSA4510C:	Straight Abutment Ø 4.5 H 1.5 JDEvolution Plus
EVNSA4520C:	Straight Abutment Ø 4.5 H 2.0 JDEvolution Plus
EVNSA4540C:	Straight Abutment Ø 4.5 H 4.0 JDEvolution Plus
EVNSA5020C:	Straight Abutment Ø 5.0 H 2.0 JDEvolution Plus
EVNSA5040C:	Straight Abutment Ø 5.0 H 4.0 JDEvolution Plus
EVNSA6020C:	Straight Abutment Ø 6.0 H 2.0 JDEvolution Plus
EVNSA6040C:	Straight Abutment Ø 6.0 H 4.0 JDEvolution Plus
EVNSA5020TSC:	Straight Abutment Tissue Ø 5.0 H 2.0 JDEvolution Plus
EVNSA5040TSC:	Straight Abutment Tissue Ø 5.0 H 4.0 JDEvolution Plus

Torque recommended 30 Ncm



Torque recommended 30 Ncm



## GP Abutment:

EV15GPAEC:	GP Abutment 15° JDEvolution Plus
EV25GPAEC:	GP Abutment 25° JDEvolution Plus
EVGPA40EC:	GP Abutment Engaging Ø 4.0 JDEvolution Plus
EVGPA40NEC:	GP Abutment Non Engaging Ø 4.0 JDEvolution Plus
EVGPAEC:	GP Abutment Engaging Ø 5.0 JDEvolution Plus
EVGPA50NEC:	GP Abutment Non Engaging Ø 5.0 JDEvolution Plus
EVGPAEPC:	GP Abutment Engaging Peek Ø 5.0 JDEvolution Plus
EVGPA60EC:	GP Abutment Engaging Ø 6.0 JDEvolution Plus

Torque recommended 30 Ncm



Torque recommended 30 Ncm



## Anatomic Abutment:

EVEA15:	Anatomic Abutment H 1.5 JDEvolution Plus
EVEA30:	Anatomic Abutment H 3.0 JDEvolution Plus
EV15A15:	15° Angulated Anatomic Abutment Ø 5.0 H 1.5 JDEvolution Plus
EV15A15N:	15° Angulated Anatomic Abutment Ø 4.5 H 1.5 JDEvolution Plus
EV15A30:	15° Angulated Anatomic Abutment Ø 5.0 H 3.0 JDEvolution Plus
EV15A30N:	15° Angulated Anatomic Abutment Ø 4.5 H 3.0 JDEvolution Plus
EV25A15:	25° Angulated Anatomic Abutment Ø 5.0 H 1.5 JDEvolution Plus
EV25A30:	25° Angulated Anatomic Abutment Ø 5.0 H 3.0 JDEvolution Plus

Torque recommended 30 Ncm



Torque recommended 30 Ncm



## Rapid Abutment:

EVRA15C:	Rapid Abutment H 1.5 JDEvolution Plus
EVRA30C:	Rapid Abutment H 3.0 JDEvolution Plus
EVRA15D:	Rapid Abutment w/o Healing Cap and Coping H 1.5 JDEvolution Plus
EVRA30D:	Rapid Abutment w/o Healing Cap and Coping H 3.0 JDEvolution Plus
EVRAHC:	Rapid Abutment Healing Cap
EVRAIC:	Rapid Abutment Impression Coping
EVRAAR:	Rapid Abutment Replica

Torque recommended 30 Ncm




Torque recommended 30 Ncm



## Wax Up Abutment:

EVWAE C:	Wax-Up Abutment Engaging JDEvolution Plus
EVWANEC:	Wax-Up Abutment Non Engaging JDEvolution Plus


Torque recommended 30 Ncm



## Cobalt-Chrome Abutment:

EVCCCE:	Chrome-Cobalt Abutment Engaging JDEvolution Plus
EVCCNEC:	Chrome-Cobalt Abutment Non Engaging JDEvolution Plus
EVCA CCNEC:	Cobalt-Chrome Conical Abutment Non Engaging JDEvolution Plus

Torque recommended 30 Ncm




15 Ncm

## Gold Abutment:




EVGAEC:	Gold Abutment Engaging JDEvolution Plus
EVGANEC:	Gold Abutment Non Engaging JDEvolution Plus

Torque recommended 30 Ncm




## Conical Abutment:

EVNCA10C:	Conical Abutment Straight H 1.0 JDEvolution Plus
EVNCA15C:	Conical Abutment Straight H 1.5 JDEvolution Plus
EVNCA20C:	Conical Abutment Straight H 2.0 JDEvolution Plus
EVNCA30C:	Conical Abutment Straight H 3.0 JDEvolution Plus
EVNCA40C:	Conical Abutment Straight H 4.0 JDEvolution Plus
EVNCA70C:	Conical Abutment Straight H 7.0 JDEvolution Plus
EVNCA90C:	Conical Abutment Straight H 9.0 JDEvolution Plus
EVNCA15TSC:	Conical Abutment Tissue Straight H 1.5 JDEvolution Plus
EVNCA30TSC:	Conical Abutment Tissue Straight H 3.0 JDEvolution Plus
EVNCA40TSC:	Conical Abutment Tissue Straight H 4.0 JDEvolution Plus
EVNCA50TSC:	Conical Abutment Tissue Straight H 5.0 JDEvolution Plus
EVCA1725C:	Conical Abutment Angulated 17° H 2.5 JDEvolution Plus
EVCA1735C:	Conical Abutment Angulated 17° H 3.5 JDEvolution Plus
EVCA3025C:	Conical Abutment Angulated 30° H 2.5 JDEvolution Plus
EVCA3035C:	Conical Abutment Angulated 30° H 3.5 JDEvolution Plus
EVCA1725TSC:	Conical Abutment Tissue Angulated 17° H 2.5 JDEvolution Plus
EVCA1735TSC:	Conical Abutment Tissue Angulated 17° H 3.5 JDEvolution Plus
EVA275C:	Conical Abutment Tissue Angulated 17° H 5.0 JDEvolution Plus
EVCA3025TSC:	Conical Abutment Tissue Angulated 30° H 2.5 JDEvolution Plus
EVCA3035TSC:	Conical Abutment Tissue Angulated 30° H 3.5 JDEvolution Plus
EVCA3050TSC:	Conical Abutment Tissue Angulated 30° H 5.0 JDEvolution Plus
EVA137C:	Conical Abutment Straight Engaging H 1.5 JDEvolution Plus
EVA138C:	Conical Abutment Straight Engaging H 3.0 JDEvolution Plus
EVS105:	Screw for Conical Abutment Straight Engaging H 1.5 JDEvolution Plus
EVS106:	Screw for Conical Abutment Straight Engaging H 3.0 JDEvolution Plus
EVCASA:	Screw for Angulated Conical Abutment JDEvolution Plus
EVCAPS:	Prosthetic Screw Conical Abutment JDEvolution Plus
EVCAPSL:	Prosthetic Screw Conical Abutment Long JDEvolution Plus
EVCAPSA	Prosthetic Screw Angulated for Conical Abutment JDEvolution
EVCAICOTEC:	Conical Abutment Impression Coping Engaging Open Tray JDEvolution Plus
EVCAICOTC:	Conical Abutment Impression Coping Open Tray JDEvolution Plus
EVCAICOTLC:	Conical Abutment Impression Coping Open Tray Long JDEvolution Plus
EVCAICOT02:	Screw for Conical Abutment Impression Coping Open Tray JDEvolution Plus
EVCAICOT04:	Screw for Conical Abutment Impression Coping Open Tray Long JDEvolution Plus
EVCAICCTC	Conical Abutment Impression Coping Closed Tray
EVCAHC:	Healing Cap for Conical Abutment JDEvolution Plus
EVCAHCL:	Conical Abutment Healing Cap H 6.0 JDEvolution Plus
EVCAHC9:	Conical Abutment Healing Cap H 9.0 JDEvolution Plus
EVCAHCB:	Conical Abutment Healing Cap Peek JDEvolution Plus
EVCAGPAEC:	GP Abutment Engaging for Conical Abutment JDEvolution Plus
EVCAGPANEC:	GP Abutment Non Engaging for Conical Abutment JDEvolution Plus
EVCATANEWSC:	Temporary Abutment Non Engaging Conical Abutment Smooth for Welding JDEvolution Plus
EVCATANEC:	Temporary Abutment Non Engaging Conical Abutment JDEvolution Plus
EVCATANEWC:	Temporary Abutment Non Engaging Conical Abutment for Welding JDEvolution Plus
EVCAWANEC:	Wax-Up Abutment Non Engaging for Conical Abutment JDEvolution Plus
EVCAAR	Conical Abutment Replica




## Conical Abutments Mini:

EVNCA10MIC:	Conical Straight Abutment MINI H 1.0 JDEvolution Plus
EVNCA15MIC:	Conical Straight Abutment MINI H 1.5 JDEvolution Plus
EVNCA30MIC:	Conical Straight Abutment MINI H 3.0 JDEvolution Plus
EVNCA40MIC:	Conical Straight Abutment MINI H 4.0 JDEvolution Plus
EVNCA50MIC:	Conical Straight Abutment MINI H 5.0 JDEvolution Plus
EVCAHCMIC:	Conical Abutment MINI Healing Cap JDEvolution Plus
EVCAHCLMIC:	Conical Abutment MINI Healing Cap H 6.0 JDEvolution Plus
EVCAITMIC:	Interface CAD CAM Non Engaging H 7.0 for Conical Abutment MINI JDEvolution Plus
EVCAITMIEC:	Interface CAD CAM Engaging H 7.0 for Conical Abutment MINI JDEvolution Plus
EVCAITBMIC:	Interface CAD CAM Non Engaging H 5.0 for Conical Abutment MINI JDEvolution Plus
EVCAITBMIEC:	Interface CAD CAM Engaging H 5.0 for Conical Abutment MINI JDEvolution Plus
EVCATANEMIC:	Temporary Abutment Non Engaging Conical Abutment MINI JDEvolution Plus
EVCAICOTMIC:	Conical Abutment MINI Impression Coping Open Tray JDEvolution Plus
EVCAICOTMIEC:	Conical Abutment MINI Impression Coping Engaging Open Tray JDEvolution Plus
EVCAARM1	Conical Abutment MINI Replica
EVCAARMIC	Conical Abutment MINI Replica CAD CAM



EVCASBCEMIC: ScanBody Conical Abutment MINI JDEvolution Plus  
 EVCASBCEMIEC: ScanBody Engaging Conical Abutment MINI JDEvolution Plus  
 EVCASBCESMIC: On Top ScanBody Conical Abutment MINI



### Prosthetic screw:

EVS: Prosthetic Screw JDEvolution Plus  
 EVSA: Prosthetic Screw Angulated JDEvolution Plus


Torque recommended 30 Ncm



### Interfaces:

EVINTEC: Interface Engaging JDEvolution Plus  
 EVINTNEC: Interface Non Engaging JDEvolution Plus  
 70287C: Interface Non Engaging for Conical Abutment JDEvolution Plus

Torque recommended 30 Ncm




15 Ncm

### AS Abutment:


EVASCEC: AS Abutment Engaging JDEvolution Plus  
 EVASCNEC: AS Abutment Non Engaging JDEvolution Plus

Torque recommended 30 Ncm



### TiBase, JDScaBody and Implant Replica CAD CAM:

EVSBCCEC: ScanBody Engaging JDEvolution Plus  
 EVCASBCEC: ScanBody Conical Abutment JDEvolution Plus  
 EVCASBCEEC: ScanBody Engaging Conical Abutment JDEvolution Plus  
 EVCASBCECSC: On Top ScanBody Conical Abutment JDEvolution Plus  
 JDSCGIOSE: ScanBody Full Arch Tracer Hexagonal  
 JDSCGIOS: ScanBody Full Arch Tracer  
 JDSCGIOSR: ScanBody Rectangular Full Arch Tracer

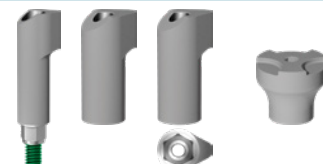

EVHSB53: On Top ScanBody Engaging Ø 5.0 H 3.0 JDEvolution Plus  
 EVHSB55: On Top ScanBody Engaging Ø 5.0 H 5.0 JDEvolution Plus  
 EVHSB57: On Top ScanBody Engaging Ø 5.0 H 7.0 JDEvolution Plus  
 EVSCPC: ScanPost JDEvolution Plus



EVTIBC: TiBase Engaging Ø4.25 H 0.5 C 4.7 JDEvolution Plus  
 EVTIBNEC: TiBase Non Engaging Ø4.25 H 0.5 C 4.7 JDEvolution Plus  
 EVTIB15C: TiBase Engaging Ø4.25 H 1.5 C 4.7 JDEvolution Plus  
 EVTIB15NEC: TiBase Non Engaging Ø4.25 H 1.5 C 4.7 JDEvolution Plus  
 EVTIB30C: TiBase Engaging Ø4.25 H 3.0 C 4.7 JDEvolution Plus  
 EVTIB30NEC: TiBase Non Engaging Ø4.25 H 3.0 C 4.7 JDEvolution Plus

Torque recommended 30 Ncm



EVTIBNC: TiBase Long Engaging Ø4.4 H 0.5 C 7.7 JDEvolution Plus  
 EVTIBNEC: TiBase Long Non Engaging Ø4.4 H 0.5 C 7.7 JDEvolution Plus  
 EVTIB10NC: TiBase New Engaging Ø4.4 H 1.0 C 7.7 JDEvolution Plus  
 EVTIB10NEC: TiBase New Non Engaging Ø4.4 H 1.0 C 7.7 JDEvolution Plus  
 EVTIB15NC: TiBase Long Engaging Ø4.4 H 1.5 C 7.7 JDEvolution Plus  
 EVTIB15NEC: TiBase Long Non Engaging Ø4.4 H 1.5 C 7.7 JDEvolution Plus  
 EVTIB20NC: TiBase New Engaging Ø4.4 H 2.0 C 7.7 JDEvolution Plus  
 EVTIB20NEC: TiBase New Non Engaging Ø4.4 H 2.0 C 7.7 JDEvolution Plus  
 EVTIB30NC: TiBase Long Engaging Ø4.4 H 3.0 C 7.7 JDEvolution Plus  
 EVTIB30NEC: TiBase Long Non Engaging Ø4.4 H 3.0 C 7.7 JDEvolution Plus

Torque recommended 30 Ncm



EVA150C: TiBase Long Engaging Ø4.4 H 0.5 C 7.7 for Angulated Channel JDEvolution Plus  
 EVA151C: TiBase New Non Engaging Ø4.4 H 0.5 C 7.7 for Angulated Channel JDEvolution Plus  
 EVA152C: TiBase Long Engaging Ø4.4 H 1.5 C 7.7 for Angulated Channel JDEvolution Plus  
 EVA153C: TiBase New Non Engaging Ø4.4 H 1.5 C 7.7 for Angulated Channel JDEvolution Plus  
 EVA154C: TiBase Long Engaging Ø4.4 H 3.0 C 7.7 for Angulated Channel JDEvolution Plus  
 EVA155C: TiBase New Non Engaging Ø4.4 H 3.0 C 7.7 for Angulated Channel JDEvolution Plus

Torque recommended 30 Ncm



EVA133C: Tibase Interface Engaging H 6.0 for Angulated Channel JDEvolution Plus\*  
 EVA134C: Tibase Interface Non Engaging H 6.0 for Angulated Channel JDEvolution Plus\*  
 EVA135C: Tibase Interface Engaging H 10.0 for Angulated Channel JDEvolution Plus\*  
 EVA136C: Tibase Interface Non Engaging H 10.0 for Angulated Channel JDEvolution Plus\*

Torque recommended 30 Ncm



EVCAITEC:	Interface CAD CAM Engaging for Conical Abutment JDEvolution Plus (H 7.5)
EVA139C:	TiBase Engaging for Conical Abutment JDEvolution Plus (H 5.0)
EVCAITC:	Interface CAD CAM Non Engaging for Conical Abutment JDEvolution Plus (H 7.3)
EVCATIBC:	TiBase for Conical Abutment JDEvolution Plus (H 5.0)
EVCAITAC:	Interface CAD CAM Non Engaging for Conical Abutment Angulated Channel (H 7.7)



EVS110:	Prosthetic Screw Conical Abutment Direct
EVS111:	Prosthetic Screw Conical Abutment Direct Long
EVS112:	Prosthetic Screw for Angulated Channel Conical Abutment Direct

Torque recommended 15 Ncm



EVANCN:	Implant Replica CAD CAM New JDEvolution Plus
EVCAARCNC:	Conical Abutment Replica CAD CAM New
EVPMNC:	Pre-milled Abutment Blank JDEvolution Plus



Torque recommended 30 Ncm



\*The EVS: prosthetic screw must be used for straight channels and the EVSA: prosthetic screw must be used for angled channels. Prosthetic screws are not included.  
**Note: please contact info@jdentalcare.com for the digital library for Exocad, 3Shape and Dental Wings software**

## Conometric Abutment:

EVCP05C:	Conometric Abutment Straight H 0.5 JDEvolution Plus
EVCP10C:	Conometric Abutment Straight H 1.0 JDEvolution Plus
EVCP20C:	Conometric Abutment Straight H 2.0 JDEvolution Plus
EVCP30C:	Conometric Abutment Straight H 3.0 JDEvolution Plus
EVCP40C:	Conometric Abutment Straight H 4.0 JDEvolution Plus
EV7CP20C:	7.5° Angulated Conometric Abutment H 2.0 JDEvolution Plus
EV15CP20C:	15° Angulated Conometric Abutment H 2.0 JDEvolution Plus
EV22CP20C:	22.5° Angulated Conometric Abutment H 2.0 JDEvolution Plus
EVA300C:	30° Angulated Conometric Abutment H 2.0 JDEvolution Plus
EVA285C:	7.5° Angulated Conometric Abutment H 3.0 JDEvolution Plus
EVA286C:	15° Angulated Conometric Abutment H 3.0 JDEvolution Plus
EVA287C:	22.5° Angulated Conometric Abutment H 3.0 JDEvolution Plus
EVA288C:	30° Angulated Conometric Abutment H 3.0 JDEvolution Plus
EVCP5:	Screw for Conometric Abutment JDEvolution Plus
EVA130C:	Cap With Pin for Intraoral Welding
EVA131C:	Cap for Partial or Full-Arch Fixed Prosthesis
EVA132C:	Anti-Rotation Cap for Single Element
EVCPIC:	Conometric Abutment Impression Coping PEEK
EVCPAN:	Conometric Abutment Replica

Torque recommended 30 Ncm



Torque recommended 30 Ncm



Torque recommended 30 Ncm




Torque recommended 30 Ncm



## Ball Abutment:

EVBA15:	Ball Abutment H 1.5 JDEvolution Plus
EVBA30:	Ball Abutment H 3.0 JDEvolution Plus
EVBA50:	Ball Abutment H 5.0 JDEvolution Plus
EVBAA:	Ball Abutment Replica
EVBAHC:	Ball Abutment Elastic Retention Cap w/Container
EVBAN:	Ball Abutment Retention Cap

Torque recommended 30 Ncm

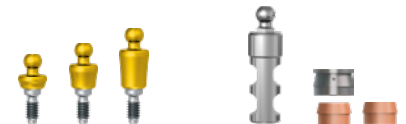

## Emi Abutment:

EVEMI15:	Emi Abutment H 1.5 JDEvolution Plus
EVEMI30:	Emi Abutment H 3.0 JDEvolution Plus
EVEMI50:	Emi Abutment H 5.0 JDEvolution Plus
EVEMISCK:	Smart cap attachment Emi Abutment
EVEMIHC:	Emi Abutment Elastic Retention Cap w/ Container
EVEMIN:	Emi Abutment Elastic Retention Cap (1.2 kg)
EVEMIH:	Emi Abutment Container
EVEMIIC:	Emi Abutment Plastic Impression Coping
EVEMIICS:	Emi Abutment Steel Impression Coping
EVEMINT:	Emi Abutment White Retention Cap (1.8 kg)
EVEMINY:	Emi Abutment Yellow Retention Cap (0.6 kg)
EVEMINP:	Emi Abutment Purple Retention Cap (2.5 kg)
EVEMINB:	Emi Abutment Retention Cap for Laboratory
EVEMIEIT:	Extractor-insertion Tool For Caps
EVEMIA:	Emi Abutment Replica

Torque recommended 30 Ncm



## Implant replica:

EVAN: Implant Replica JDEvolution Plus



## Bone Mill:

JDBMNC: Bone Mill Ø 5.0 and Guide JDEvolution Plus  
 JDBM6NC: Bone Mill Ø 6.0 and Guide JDEvolution Plus  
 JDBMGNN: Bone Mill Guide JDEvolution Plus




## Short Drills:

JDDICS4 Short Drill Ø 4mm L 6 JDIcon Plus  
 JDDICS4D Short Drill Ø 4mm L 6 Dense Bone JDIcon Plus  
 JDDICS5 Short Drill Ø 5mm L 6 JDIcon Plus



## Implant and Prosthetic Drivers:

EVID: Implant Driver JDEvolution Plus  
 EVIDL: Implant Driver Long JDEvolution Plus  
 JDID127 Implant Depth Aligner JDEvolution Plus  
 EVSDPF15: Prosthetic Driver for JDTorque L 15 JDEvolution Plus  
 EVSDPF20: Prosthetic Driver for JDTorque L 20 JDEvolution Plus  
 EVSDPF25: Prosthetic Driver for JDTorque L 25 JDEvolution Plus  
 EVSDPF35: Prosthetic Driver for JDTorque L 35 JDEvolution Plus  
 EVSDPF60: Prosthetic Driver for JDTorque L 60 JDEvolution Plus  
 EVSDCAF Conical Abutment Driver for JDTorque  
 EVSDP20: Prosthetic Driver L 20 JDEvolution Plus  
 EVSDP25: Prosthetic Driver L 25 JDEvolution Plus  
 EVSDP30: Prosthetic Driver L 30 JDEvolution Plus  
 JDPD105 Prosthetic Driver JDEvolution Plus for Surgical Driver  
 EVSDCA Conical Abutment Driver  
 EVSDPF25A Angulated Screw Driver for JDTorque L 25  
 EVSDPF30A Angulated Screw Driver for JDTorque L 30  
 EVSDPF25AV Angulated Screw Driver for Conical Abutment Direct JDTorque L 25  
 EVSDPF30AV Angulated Screw Driver for Conical Abutment Direct JDTorque L 30  
 EVSDP32AV Screw Driver for Conical Abutment Direct EVS112 (Straight Channel)  
 EVSUD Surgical Driver JDEvolution  
 JDG JDGuide  
 EVGMC Implant Mounter for JDEvolution  
 EVGMLC Implant Mounter Long JDEvolution  
 JDID102 ZAPA Tool  
 JDSRP Dental Implant Depth Probe

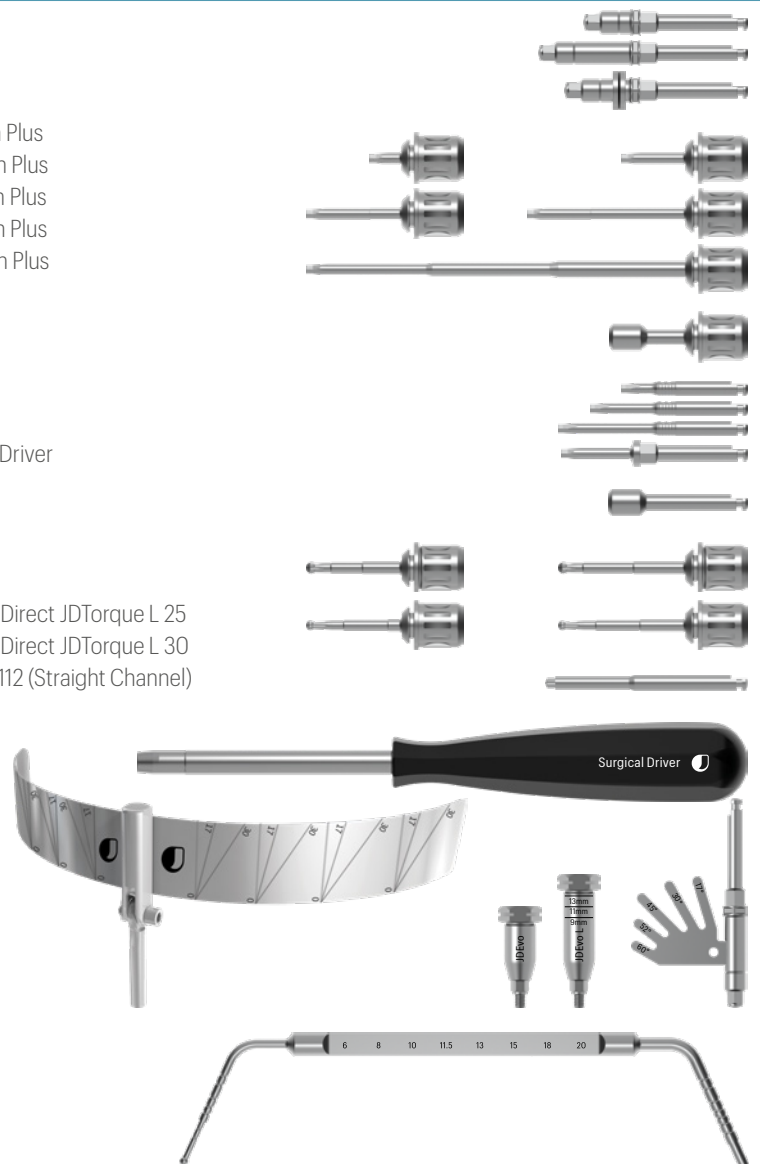





## Direction indicators:

JDDI Direction Indicator  
 JDDIS Direction Indicator Short  
 JDDI17 Direction Indicator 17°  
 JDDI30 Direction Indicator 30°  
 JDDI45 Direction Indicator 45°



# DRILLING PROTOCOLS

It is recommended to adhere to the indications of the following drilling sequence to ensure optimal primary stability of the implants

IMPLANT DIAMETER	HEALED BONE		POST EXTRACTIVE BONE		
	SOFT BONE	MEDIUM-DENSE BONE	SOFT BONE	MEDIUM-DENSE BONE	
<b>site preparation in maxilla</b>					
<b>Ø 3,7</b>	2,0 2,4 2,8 up to the 1 <sup>st</sup> laser mark L6mm	2,0 2,4 2,8 3,2 up to the 1 <sup>st</sup> laser mark L6mm	2,0 2,4 2,8 at the entrance	2,0 2,4 2,8 at the entrance	  <p>Short Implant L 6mm JDEvolution Plus insertion in maxilla</p>
	<b>Ø 4,0</b>	2,0 2,4 2,8 up to the 1 <sup>st</sup> laser mark L6mm	2,0 2,4 2,8 3,2 up to the 1 <sup>st</sup> laser mark L6mm	2,0 2,4 2,8 at the entrance	
<b>Ø 4,3</b>		2,0 2,4 2,8 3,2 at the entrance	2,0 2,4 2,8 3,2 up to the 1 <sup>st</sup> laser mark L6-8mm 3,6 at the entrance	2,0 2,4 2,8 3,2 at the entrance	2,0 2,4 2,8 3,2 at the entrance
	<b>Ø 5,0</b>	2,0 2,4 2,8 3,2 3,6 up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 up to the 1 <sup>st</sup> laser mark L 6mm 4,0 at the entrance	2,0 2,4 2,8 3,2 3,6 at the entrance up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 at the entrance up to the 1 <sup>st</sup> laser mark L 6mm
<b>Ø 6,0</b>		2,0 2,4 2,8 3,2 3,6	2,0 2,4 2,8 3,2 3,6 4,0 4,4 4,8 up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 4,0	2,0 2,4 2,8 3,2 3,6 4,0
	<b>site preparation in mandible</b>				
<b>Ø 3,7</b>	2,0 2,4 2,8 3,2 up to the 2 <sup>nd</sup> laser mark L 8mm 3,6 up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 at the entrance	2,0 2,4 2,8 3,2 at the entrance	  <p>Short Implant L 6mm JDEvolution Plus insertion in mandible</p>
	<b>Ø 4,0</b>	2,0 2,4 2,8 3,2 up to the 2 <sup>nd</sup> laser mark L 8mm 3,6 up to the 1 <sup>st</sup> laser mark L 6mm 4,0 up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 up to the 1 <sup>st</sup> laser mark L 6mm 4,0 up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 up to the 1 <sup>st</sup> laser mark L 6mm 3,6 up to the 1 <sup>st</sup> laser mark L 6mm	
<b>Ø 4,3</b>		2,0 2,4 2,8 3,2 3,6 up to the 2 <sup>nd</sup> laser mark L 8mm 4,0 up to the 2 <sup>nd</sup> laser mark L 8mm	2,0 2,4 2,8 3,2 3,6 4,0 up to the 2 <sup>nd</sup> laser mark L8mm 4,4 up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 at the entrance	2,0 2,4 2,8 3,2 3,6 at the entrance
	<b>Ø 5,0</b>	2,0 2,4 2,8 3,2 3,6 4,0 4,4 up to the 2 <sup>nd</sup> laser mark L 8mm 4,8 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 4,4 4,8 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 at the entrance
<b>Ø 6,0</b>		2,0 2,4 2,8 3,2 3,6 4,0 4,4 4,8 up to the 1 <sup>st</sup> laser mark L 6mm 5,4 up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 4,0 4,4 4,8 up to the 2 <sup>nd</sup> laser mark L 8mm 5,4 up to the 2 <sup>nd</sup> laser mark L 8mm	2,0 2,4 2,8 3,2 3,6 4,0 4,4	2,0 2,4 2,8 3,2 3,6 4,0 4,4


Note: All measurements in mm

# DRILLING PROTOCOLS - Ø 4,0 T IMPLANTS

It is recommended to adhere to the indications of the following drilling sequence to ensure optimal primary stability of the implants.

IMPLANT DIAMETER	HEALED BONE		POST EXTRACTIVE BONE		
	SOFT BONE	MEDIUM-DENSE BONE	SOFT BONE	MEDIUM-DENSE BONE	
<b>site preparation in maxilla</b>					Short Implant L 6mm JDEvolution Plus insertion in maxilla
Ø 4,0	2.0	2.0	2.0	2.0	<b>short Ø 4,0 L 6</b> - Start the osteotomy with standard twist drill Ø 2.0mm and Ø 2.4mm - Complete with the Ø 4mm L 6mm drill code JDDICS4
	2.4	2.4	2.4	2.4	
	2.8	2.8 3.2 up to the 2 <sup>nd</sup> laser mark L 8mm	2.8 up to the 2 <sup>nd</sup> laser mark L 8mm	2.8	
<b>site preparation in mandible</b>					Short Implant L 6mm JDEvolution Plus insertion in mandible
Ø 4,0	2.0	2.0	2.0	2.0	<b>short Ø 4,0 L 6</b> - Start the osteotomy with standard twist drill Ø 2.0mm, Ø 2.4mm and Ø 2.8mm - Complete with the Ø 4mm L 6mm drill code JDDICS4D
	2.4	2.4	2.4	2.4	
	2.8	3.2 up to the 2 <sup>nd</sup> laser mark L 8mm 3.6 up to the 2 <sup>nd</sup> laser mark L 8mm	2.8 3.2 up to the 2 <sup>nd</sup> laser mark L 8mm 3.6 up to the 2 <sup>nd</sup> laser mark L 8mm	2.8 3.2 3.6 up to the 2 <sup>nd</sup> laser mark L 8mm	

Note: all measurements in mm

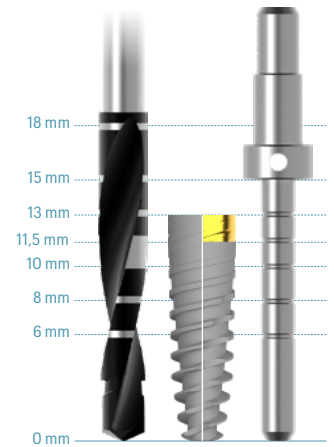



**JDENTALCARE**

[www.jdentalcare.com](http://www.jdentalcare.com)

JDentalCare, the JDentalCare logo and other trademarks mentioned in this document are, excluding specifically mentioned exceptions, trademarks property of JDentalCare.

The images of the products represented in this brochure are not necessarily to scale.

Note: Not all products manufactured by JDentalCare and represented in this brochure have been regulatory cleared/released for sale in all countries and/or have been licensed in accordance with FDA Rules and Regulations.

For more information about current product assortment and availability, please contact your local JDentalCare distributor. For prescription only.

Caution: Federal (US) law restricts this device to sale by or on the order for a licensed dentist.

See instructions for use for more information such as indications, warnings, precaution and contraindications.

EVPCAT  
REV.67 of 2026-02-12