




J DENTAL CARE  
*just smile*

# JD ICON

*The unique features of an icon*



conical connection



Made in Italy

## THE CONICAL CONNECTION

The conical connection offers:


- Tight seal and high mechanical strength
- High level of mechanical stability under different load conditions
- Better force transition from the implant body to the prosthetic abutment
- Less stress on the prosthetic screw

The conical connection is significantly **superior in term of bacterial seal** as compared to other connection systems and it is more resistant to abutment movement and microgap enlargement under loading.

The internal conical connection also allows for platform shifting, allowing the preservation of the crestal bone and the volume of the surrounding soft tissue. This results in more **natural looking gums** and also supports **less radiographically detectable crestal bone loss**.

Whereas with other connections, platform shifting is achieved through the use of a smaller diameter abutment on a larger diameter implant collar, the internal conical connection has the shift built-in.

The hexagonal interlocking provides a choice of six different abutment positions providing **high restorative flexibility**.

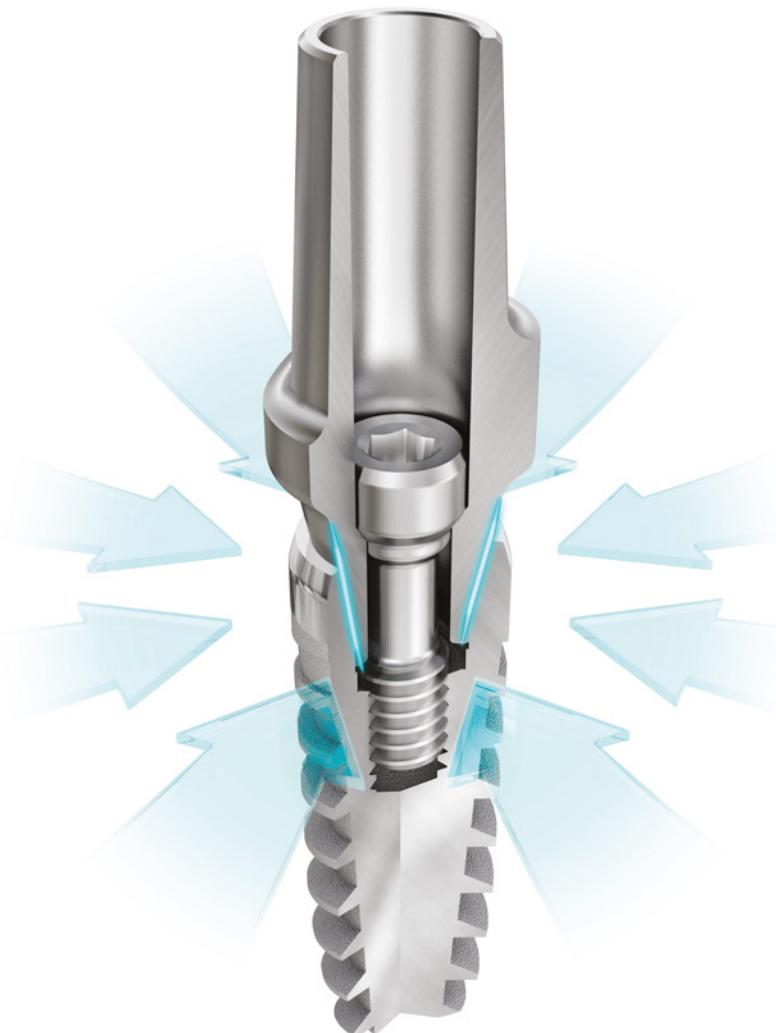

## SINGLE PROSTHETIC CONNECTION

### features

- Single prosthetic connection for all diameters
- Dual system conical connection internal hexagonal
- Built-in platform switching
- Complete selection of temporary and final abutments for various heights and emergence profiles

### JDICON



### JDICON F

### advantages

- Simplicity of clinical processes
- Reduces inventory and enhanced working flexibility
- Excellent connection stability
- Sealed connection: thanks to the connection design, there are no detectable microgaps at the implant-abutment in the area of the conical connection
- High mechanical strength
- Greater hard and soft tissue stability

## THE UNIQUE FEATURES OF AN ICON

### features

#### JDICON

Available with 1.5 mm machined implant collar or fully treated without machined implant collar

Machined implant collar

Expanding tapered inner body

Self-cutting capacity in both directions

Apical cutting blades

#### JDICON F

#### JDICON F

Wide product range to meet the needs of all surgical situations

Reduces the risk of perimplantitis. Allows the placement of the top of the implant above the alveolar crest to make distance between the abutment-fixture microgap and the bone reducing bone loss

Favours gradual condensation of bone and guarantees high primary stability, especially in compromised bone situations

Makes it possible to achieve high primary stability with low torque


They allow the implant to engage osteotomies

## PRODUCT SPECIFICATIONS

The JDIcon dental implants are available in the diameters and lengths shown in the following table:

IMPLANT DIAMETER	LENGTH	TIP DIAMETER	PLATFORM DIAMETER	ABUTMENT INTERFACE
<b>Ø 3,9</b>	8	2.5	3.9	3.4
	10, 11.5	2.4		
	13, 15, 18, 20	2.8		
<b>Ø 4,3</b>	6, 8	3.25	4	3.4
	10, 11.5, 13, 15	2.8		
<b>Ø 5,0</b>	6, 8, 10, 11.5, 13, 15	3.2	4.7	3.4

Note: all measurements in mm

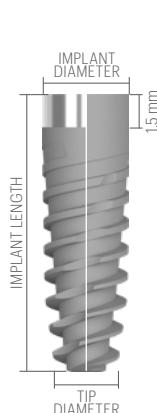

# PRODUCT CATALOGUE

## JDIcon with 1.5mm machined implant collar:

### Ø 3,9

IC39080	JDIcon Ø 3.9 L 8
IC39100	JDIcon Ø 3.9 L 10
IC39115	JDIcon Ø 3.9 L 11.5
IC39130	JDIcon Ø 3.9 L 13
IC39150	JDIcon Ø 3.9 L 15
IC39180	JDIcon Ø 3.9 L 18
IC39200	JDIcon Ø 3.9 L 20



### Ø 4,3

IC43060	JDIcon Ø 4.3 L 6
IC43080	JDIcon Ø 4.3 L 8
IC43100	JDIcon Ø 4.3 L 10
IC43115	JDIcon Ø 4.3 L 11.5
IC43130	JDIcon Ø 4.3 L 13
IC43150	JDIcon Ø 4.3 L 15



### Ø 5,0


IC50060	JDIcon Ø 5.0 L 6
IC50080	JDIcon Ø 5.0 L 8
IC50100	JDIcon Ø 5.0 L 10
IC50115	JDIcon Ø 5.0 L 11.5
IC50130	JDIcon Ø 5.0 L 13
IC50150	JDIcon Ø 5.0 L 15



## JDIcon F fully treated:

### Ø 3,9

IC39080:	JDIcon F Ø 3.9 L 8
IC39100:	JDIcon F Ø 3.9 L 10
IC39115:	JDIcon F Ø 3.9 L 11.5
IC39130:	JDIcon F Ø 3.9 L 13
IC39150:	JDIcon F Ø 3.9 L 15
IC39180:	JDIcon F Ø 3.9 L 18
IC39200:	JDIcon F Ø 3.9 L 20

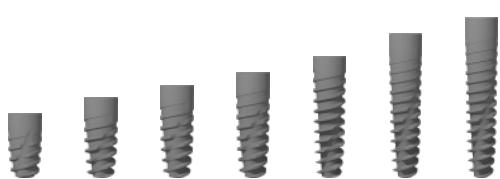


### Ø 4,3

IC43060:	JDIcon F Ø 4.3 L 6
IC43080:	JDIcon F Ø 4.3 L 8
IC43100:	JDIcon F Ø 4.3 L 10
IC43115:	JDIcon F Ø 4.3 L 11.5
IC43130:	JDIcon F Ø 4.3 L 13
IC43150:	JDIcon F Ø 4.3 L 15



### Ø 5,0

IC50060:	JDIcon F Ø 5.0 L 6
IC50080:	JDIcon F Ø 5.0 L 8
IC50100:	JDIcon F Ø 5.0 L 10
IC50115:	JDIcon F Ø 5.0 L 11.5
IC50130:	JDIcon F Ø 5.0 L 13
IC50150:	JDIcon F Ø 5.0 L 15

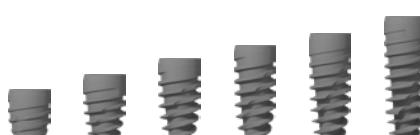

## Cover Screw:

ICCS	Cover Screw JDIcon
------	--------------------



## Healing Abutment:

ICHA43	Healing Abutment Ø 4.0 H 3.0 JDIcon
ICHA45	Healing Abutment Ø 4.0 H 5.0 JDIcon
ICHA47	Healing Abutment Ø 4.0 H 7.0 JDIcon
ICHA53	Healing Abutment Ø 5.0 H 3.0 JDIcon
ICHA55	Healing Abutment Ø 5.0 H 5.0 JDIcon
ICHA57	Healing Abutment Ø 5.0 H 7.0 JDIcon
ICHA59	Healing Abutment Ø 5.0 H 9.0 JDIcon
ICHA63	Healing Abutment Ø 6.0 H 3.0 JDIcon
ICHA65	Healing Abutment Ø 6.0 H 5.0 JDIcon
ICHA67	Healing Abutment Ø 6.0 H 7.0 JDIcon



## Healing Abutments Bridge:


ICHA53B	Healing Abutment Bridge Ø 5.0 H 3.0 JDIcon
ICHA55B	Healing Abutment Bridge Ø 5.0 H 5.0 JDIcon
ICHA57B	Healing Abutment Bridge Ø 5.0 H 7.0 JDIcon



## Impression Coping:

### OPEN TRAY

ICICOT4C	Impression Coping Open Tray Ø 4.0 JDIcon
ICICOT5C	Impression Coping Open Tray Ø 5.0 JDIcon
ICICOT6C	Impression Coping Open Tray Ø 6.0 JDIcon



### CLOSED TRAY

ICICCT4C	Impression Coping Closed Tray Ø 4.0 JDIcon
ICICCT5C	Impression Coping Closed Tray Ø 5.0 JDIcon
ICICCT6C	Impression Coping Closed Tray Ø 6.0 JDIcon

## Impression Coping Bridge:

ICICOTNEC	Impression Coping Open Tray for Bridge JDIcon
-----------	---



## Temporary Abutment:

ICTAEC	Temporary Abutment Engaging JDIcon
ICTANEC	Temporary Abutment Non Engaging JDIcon
ICA100	Temporary Abutment Engaging H 3.0 JDIcon
ICATANEWC	Temporary Abutment Non Engaging for Welding JDIcon

Torque recommended 30 Ncm



## Straight Abutment:

ICSA4520C	Straight Abutment Ø 4.5 H 2.0 JDIcon
ICSA4540C	Straight Abutment Ø 4.5 H 4.0 JDIcon
ICSA5020C	Straight Abutment Ø 5.0 H 2.0 JDIcon
ICSA5040C	Straight Abutment Ø 5.0 H 4.0 JDIcon
ICSA6020C	Straight Abutment Ø 6.0 H 2.0 JDIcon
ICSA6040C	Straight Abutment Ø 6.0 H 4.0 JDIcon

Torque recommended 30 Ncm



## GP Abutment:

ICGP40C	GP Abutment Ø 4.0 JDIcon
ICGP50C	GP Abutment Ø 5.0 JDIcon
ICGP60C	GP Abutment Ø 6.0 JDIcon

Torque recommended 30 Ncm



## Anatomic Abutment:

ICEA15C	Anatomic Abutment H 1.5 JDIcon
ICEA30C	Anatomic Abutment H 3.0 JDIcon
IC15A15C	15° Angulated Anatomic Abutment Ø 5.5 H 1.5 JDIcon
IC15A30C	15° Angulated Anatomic Abutment Ø 5.5 H 3.0 JDIcon
IC25A15C	25° Angulated Anatomic Abutment Ø 5.5 H 1.5 JDIcon
IC25A30C	25° Angulated Anatomic Abutment Ø 5.5 H 3.0 JDIcon

Torque recommended 30 Ncm



## Wax-Up Abutment:

ICWAEC	Wax-Up Abutment Engaging JDIcon
ICWANEC	Wax-Up Abutment Non Engaging JDIcon

Torque recommended 30 Ncm



## Gold Abutment:

ICGAEC	Gold Abutment Engaging JDIcon
ICGANEC	Gold Abutment Non Engaging JDIcon

Torque recommended 30 Ncm



## Prosthetic Screw:

ICS	Prosthetic Screw JDIcon
ICSA	Prosthetic Screw Angulated JDIcon

Torque recommended 30 Ncm



## Abutment Retrieval Tool:




ICATR	Abutment Retrieval Tool JDIcon
-------	--------------------------------



## Conical Abutment:

ICCA15C	Conical Abutment H 1.5 JDIcon	Torque recommended 30 Ncm	
ICCA30C	Conical Abutment H 3.0 JDIcon	Torque recommended 30 Ncm	
ICCA1725C	Conical Abutment Angulated 17° H 2.5 JDIcon	Torque recommended 30 Ncm	
ICCA1735C	Conical Abutment Angulated 17° H 3.5 JDIcon	Torque recommended 30 Ncm	
ICCA3025C	Conical Abutment Angulated 30° H 2.5 JDIcon	Torque recommended 30 Ncm	
ICCA3035C	Conical Abutment Angulated 30° H 3.5 JDIcon	Torque recommended 30 Ncm	
ICCASA	Conical Abutment Angulated Screw JDIcon	Torque recommended 30 Ncm	
EVCAPI	Prosthetic Screw Conical Abutment JDEvolution	Torque recommended 30 Ncm	
EVCAPI	Prosthetic Screw Angulated for Conical Abutment JDEvolution	Torque recommended 15 Ncm	
EVCAICOTEC	Conical Abutment Impression Coping Open Tray Engaging JDEvolution	Torque recommended 15 Ncm	
EVCAICOTC	Conical Abutment Impression Coping Open Tray JDEvolution	Torque recommended 15 Ncm	
EVCAICOTLC	Conical Abutment Impression Coping Open Tray Long JDEvolution	Torque recommended 15 Ncm	
EVCAICOT02	Screw for Conical Abutment Impression Coping Open Tray JDEvolution	Torque recommended 15 Ncm	
EVCAICOT04	Screw for Conical Abutment Impression Coping Open Tray Long JDEvolution	Torque recommended 15 Ncm	
EVCAICCTC	Conical Abutment Impression Coping Closed Tray	Torque recommended 15 Ncm	
EVCAHC	Conical Abutment Healing Cap JDEvolution	Torque recommended 15 Ncm	
EVCAHCL	Conical Abutment Healing Cap H 6.0 JDEvolution	Torque recommended 15 Ncm	
EVCAHC9	Conical Abutment Healing Cap H 9.0 JDEvolution	Torque recommended 15 Ncm	
EVCAHCB	Conical Abutment Healing Cap Peek JDEvolution	Torque recommended 15 Ncm	
EVCAPI	GP Abutment Engaging for Conical Abutment JDEvolution	Torque recommended 15 Ncm	
EVCAPI	GP Abutment Non Engaging for Conical Abutment JDEvolution	Torque recommended 15 Ncm	
EVCAPI	Temporary Abutment Non Engaging Conical Abutment JDEvolution	Torque recommended 15 Ncm	
EVCAPI	Temporary Abutment Non Engaging Conical Abutment JDEvolution	Torque recommended 15 Ncm	
EVCAPI	Temporary Abutment Non Engaging Conical Abutment Smooth for Welding JDEvolution	Torque recommended 15 Ncm	
EVCAPI	Wax-Up Abutment Non Engaging for Conical Abutment	Torque recommended 15 Ncm	
EVCAAR	Conical Abutment Replica	Torque recommended 15 Ncm	

## TiBase, JDScanBody and Implant Replica CAD CAM:

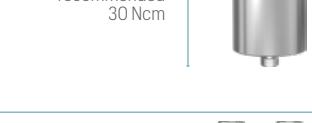ICSBCEC	ScanBody Engaging JDIcon		
EVCAEBCEC	ScanBody Conical Abutment JDEvolution		
EVCAEBCEC	ScanBody Engaging Conical Abutment JDEvolution Plus		
JDSCGIOSE	On Top ScanBody Conical Abutment JDEvolution Plus*		
JDSCGIOS	ScanBody Full Arch Tracer Hexagonal		
JDSCGIOSR	ScanBody Full Arch Tracer		
ICTIBC	ScanBody Rectangular Full Arch Tracer		
ICTIBNEC	TiBase Engaging Ø4.5 H 0.5 C 4.7 JDIcon		
ICTIB15C	TiBase Non Engaging Ø4.5 H 0.5 C 4.7 JDIcon		
ICTIB15NEC	TiBase engaging Ø4.5 H 1.5 C 4.7 JDIcon		
ICTIB30C	TiBase non engaging Ø4.5 H 1.5 C 4.7 JDIcon		
ICTIB30NEC	TiBase engaging Ø4.5 H 3.0 C 4.7 JDIcon		
EVCAITEC	TiBase non engaging Ø4.5 H 3.0 C 4.7 JDIcon		
EVA139C	Interface CAD CAM for Conical Abutment Engaging JDEvolution (H 7.5)		
EVCAITC	TiBase Engaging for Conical Abutment (H 5.0)		
EVCAITC	Interface CAD CAM for Conical Abutment Non Engaging JDEvolution (H 7.3)		
EVCAITAC	TiBase for Conical Abutment JDEvolution (H 5.0)		
EVCAITAC	Interface CAD CAM Non Engaging for Conical Abutment Angulated Channel (H 7.7)		
EVS110	Prosthetic Screw Conical Abutment Direct		
EVS111	Prosthetic Screw Conical Abutment Direct Long		
EVS112	Prosthetic Screw for Angulated Channel Conical Abutment Direct		
ICANCN	Implant Replica CAD CAM New JDIcon		
EVCAARCN	Conical Abutment Replica CAD CAM New		
ICPMNC	Pre-milled Abutment Blank JDIcon		

\*Use JDEvolution Plus screwdriver for screwing

## Interfaces:

ICINTEC	Interface Engaging JDIcon		
ICINTNEC	Interface Non Engaging JDIcon		

## Ball Abutment:

ICBA15	Ball Abutment H 1.5 JDIcon	Torque recommended 30 Ncm	
ICBA30	Ball Abutment H 3.0 JDIcon	Torque recommended 30 Ncm	
ICBA50	Ball Abutment H 5.0 JDIcon	Torque recommended 30 Ncm	
EVBA	Ball Abutment Replica	Torque recommended 30 Ncm	
EVBAHC	Ball Abutment Elastic Retention Cap w/ Container	Torque recommended 30 Ncm	
EVBAN	Ball Abutment Retention Cap	Torque recommended 30 Ncm	

## Emi Abutment:

ICEMI15	Emi Abutment H 1.5 JDIcon
ICEMI30	Emi Abutment H 3.0 JDIcon
ICEMI50	Emi Abutment H 5.0 JDIcon
EVEMISCK	Smart cap attachment Emi Abutment
EVEMIHC	Emi Abutment Elastic Retention Cap w/ Container
EVEMIN	Emi Abutment Elastic Retention Cap (1.2 kg)
EVEMIH	Emi Abutment Container
EVEMIIC	Emi Abutment Plastic Impression Coping
EVEMIICS	Emi Abutment Steel Impression Coping
EVEMINT	Emi Abutment White Retention Cap (1.8 kg)
EVEMINY	Emi Abutment Yellow Retention Cap (0.6 kg)
EVEMINP	Emi Abutment Purple Retention Cap (2.5 kg)
EVEMINB	Emi Abutment Retention Cap for Laboratory
EVEMIEIT	Extractor-insertion Tool For Caps
EVEMIA	Emi Abutment Replica

Torque recommended 30 Ncm



## Implant Replica:

ICAN	Implant Replica JDIcon
------	------------------------



## Implant and Prosthetic Drivers:

ICID	Implant Driver JDIcon
ICIDL	Implant Driver Long JDIcon
EVSDPF15	Prosthetic Driver for JDTorque L 15
EVSDPF20	Prosthetic Driver for JDTorque L 20
EVSDPF25	Prosthetic Driver for JDTorque L 25
EVSDPF35	Prosthetic Driver for JDTorque L 35
EVSDPF60	Prosthetic Driver for JDTorque L 60
EVSDCAF	Conical Abutment Driver for JDTorque
EVSDP20	Prosthetic Driver L 20
EVSDP25	Prosthetic Driver L 25
EVSDP30	Prosthetic Driver L 30
JDPD103	Prosthetic Driver for Surgical Driver
EVSDCA	Conical Abutment Driver
EVSDPF25A	Angulated Screw Driver for JDTorque L 25
EVSDPF30A	Angulated Screw Driver for JDTorque L 30
EVSDPF25AV	Angulated Screw Driver for Conical Abutment Direct JDTorque L 25
EVSDPF30AV	Angulated Screw Driver for Conical Abutment Direct JDTorque L 30
EVSDP32AV	Screw Driver for Conical Abutment Direct EVS112 (Straight Channel)
EVSUD	Surgical Driver JDEvolution
JDG	JDGuide
ICGMC	Implant Mounter for JDIcon



## Direction indicators:

JDDI	Direction Indicator
JDDIS	Direction Indicator Short
JDDI17	Direction Indicator 17°
JDDI30	Direction Indicator 30°
JDDI45	Direction Indicator 45°




# DRILLING PROTOCOLS

It is recommended to adhere to the indications of the following drilling sequence to ensure optimal primary stability of the implants

IMPLANT DIAMETER	HEALED BONE		POST EXTRACTIVE BONE		short Ø 4,3 L 6	short Ø 5,0 L 6
	SOFT BONE	MEDIUM-DENSE BONE	SOFT BONE	MEDIUM-DENSE BONE		
<b>site preparation in maxilla</b>						
Ø 3,9	2,0 2,4 2,8 up to the 1 <sup>st</sup> laser mark L6mm	2,0 2,4 2,8 3,2 up to the 1 <sup>st</sup> laser mark L6mm	2,0 2,4 2,8 at the entrance	2,0 2,4 2,8 at the entrance		
Ø 4,3	2,0 2,4 2,8 3,2 at the entrance	2,0 2,4 2,8 3,2 up to the 1 <sup>st</sup> laser mark L6-8mm 3,6 at the entrance	2,0 2,4 2,8 3,2 at the entrance	2,0 2,4 2,8 3,2 at the entrance		
Ø 5,0	2,0 2,4 2,8 3,2 3,6 up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 up to the 1 <sup>st</sup> laser mark L 6mm 4,0 at the entrance	2,0 2,4 2,8 3,2 3,6 at the entrance up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 at the entrance up to the 1 <sup>st</sup> laser mark L 6mm		
<b>site preparation in mandible</b>						
Ø 3,9	2,0 2,4 2,8 3,2 up to the 2 <sup>nd</sup> laser mark L 8mm 3,6 up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 at the entrance	2,0 2,4 2,8 3,2 at the entrance		
Ø 4,3	2,0 2,4 2,8 3,2 3,6 up to the 2 <sup>nd</sup> laser mark L 8mm 4,0 up to the 2 <sup>nd</sup> laser mark L 8mm	2,0 2,4 2,8 3,2 3,6 4,0 up to the 2 <sup>nd</sup> laser mark L 8mm 4,4 up to the 1 <sup>st</sup> laser mark L 6mm	2,0 2,4 2,8 3,2 3,6 at the entrance	2,0 2,4 2,8 3,2 3,6 at the entrance		
Ø 5,0	2,0 2,4 2,8 3,2 3,6 4,0 4,4 up to the 2 <sup>nd</sup> laser mark L 8mm 4,8 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 4,4 up to the 2 <sup>nd</sup> laser mark L 8mm 4,8 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 at the entrance	2,0 2,4 2,8 3,2 3,6 4,0 at the entrance		


Note: All measurements in mm



Short Implant L 6mm  
JDIcon insertion in maxilla



Short Implant L 6mm JDIcon insertion in mandible

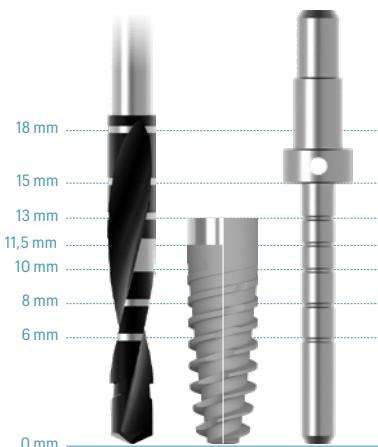

JDentalCare, the JDentalCare logo and other trademarks mentioned in this document are, excluding specifically mentioned exceptions, trademarks property of JDentalCare.

The images of the products represented in this brochure are not necessarily to scale.

Note: Not all products manufactured by JDentalCare and represented in this brochure have been regulatory cleared/released for sale in all countries and/or have been licensed in accordance with FDA Rules and Regulations.

For more information about current product assortment and availability, please contact your local JDentalCare distributor. For prescription only.

Caution: Federal (US) law restricts this device to sale by or on the other for a licensed dentist.

See instructions for use for more information such as indications, warnings, precaution and contraindications.